


## Summary of the first application

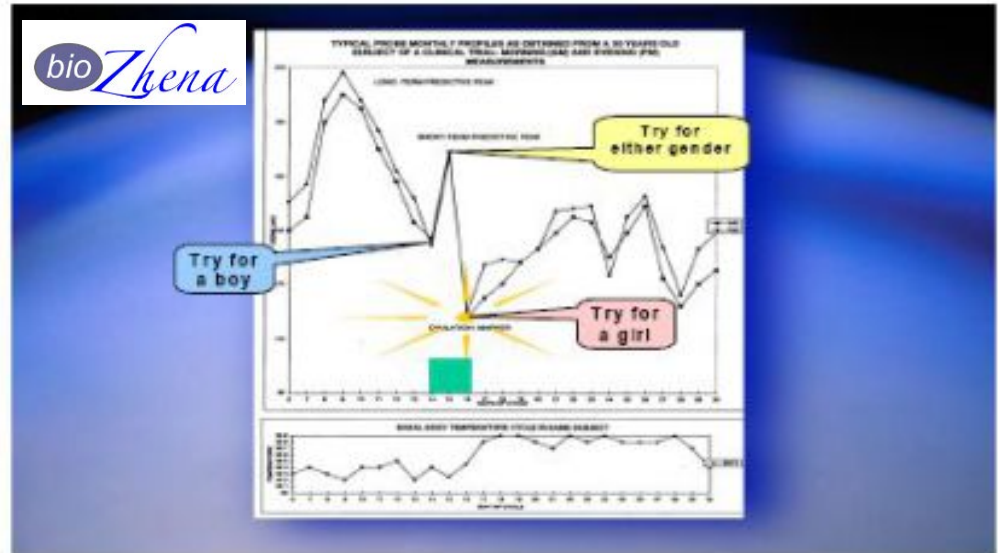

*The personal home-use device determines the 3 days during which conception can occur, and it generates a new type of profile for use by the medical profession*

Citing from FDA 510K Letter Number K973860: ... *The Monitor serves as an independent information aid to the woman by helping her to define the fertile window... whereby she may choose the proper timing for vaginal intercourse. ... The Monitor may serve to provide the user and her physician with data to better time artificial insemination or other interventional techniques.*